



Gas



Liquid & Slurry



Solid & Powder



Steam & Water

# SENTRY MVD SAMPLER

## Low Emission Samplers

### MANUAL SAMPLING

The Sentry® MVD manual low emission sampler is ideal for sampling liquids in a closed loop in refining, chemical, petrochemical and nuclear applications without emissions or exposure to the operator. The double block valve configuration assures an extra degree of safety for operators, minimizing dead volume with its unique design. The speed loop guarantees representative sample availability at the valve at all times.

For nuclear applications, the Sentry MVD sampler normally is used to collect primary side (RCS) samples for laboratory analysis. However, it also can be used to collect samples on secondary side (PWR) or turbine building side (BWR).

#### MODELS

Sentry MVD

#### BENEFITS

The Sentry MVD sampler provides representative samples while protecting the safety of operators and the environment.

The Sentry MVD sampler features a side-discharge dual needle assembly that ensures septum integrity and full venting of process vapors. This non-coring needle punctures the septum without coring it, allowing for full resealing of the septum when the sample bottle is removed. The tapered bottle shroud enables proper septum and needle alignment, preventing accidental spillage or needle breakage.

A variety of needle arrangements and sample bottle sizes are available to meet most sampling requirements. Additionally, a tube stub option is available for high viscosity fluids or slurries that contain particulates.

Since operator safety is of the highest concern, the sampling valve interface features an adjustable throttle stop and spring-loaded (dead man's) throttling valve. This provides proper sample control and quick closure upon release of the sampling valve.

#### FEATURES

- Non-coring needle design improves septum integrity
- Spring-loaded shut-off valve helps to protect against over-filling
- Separate fill and vent needles reliably vent vapors
- Unique double block valve configuration adds safety
- Needle assembly requires simple replacement without replacement of valve or disconnection of piping/tubing
- Optional nitrogen purge connection for cleaning of needles assures representative sample
- Variety of sizes and configurations available to meet various application needs
- Options include: panel-mounted valves for floor-standing or wall-mounted installations; special elastomers; NPT, SW, and metric connections; 1/2-inch valved units; isolation valves; coolers




Sample. Monitor. Measure.



# SENTRY

Any Application. Anywhere.

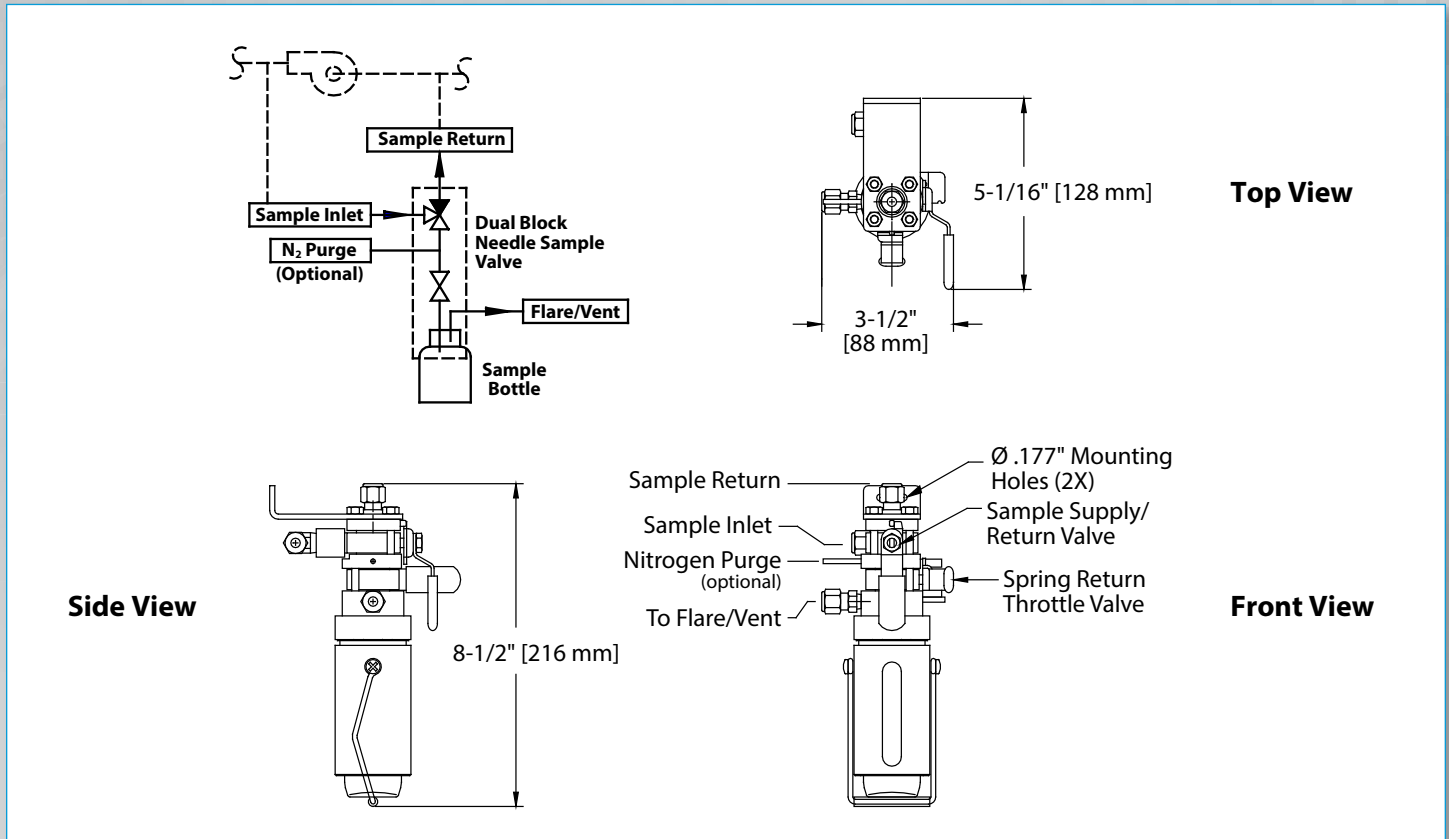

**SPECIFICATIONS**

wetted materials	316 stainless steel, PTFE, Viton®, Kalrez®				
bottle shroud	nylon				
customer interface connection	1/4 in compression, 3/8 in compression or 1/2 in compression				
standard pressure rating	1000 psi at 250°F (70 bar at 122°C); 450°F max at 100 psi (232°C at 7 bar)				
sampler interface	needle assembly (OD)*		bottle size and type	Boston round	Schott
	process	vent		2 oz (60 ml)	50 ml
	0.065 in	0.065 in	4 oz (125 ml)	100 ml	
	0.083 in	0.083 in	8 oz (250 ml)	250 ml	
	0.110 in	0.110 in	16 oz (500 ml)	500 ml	
	tube stub assembly (OD)		32 oz (1000 ml)	2000 ml	
	process	vent			
	3/16 in	9/64 in			

\*other needle/tube stub arrangements available

Boston Round bottle cap/thread interfaces per GPI finish standards. Schott/Duran bottle cap/thread interfaces per ISO 4796. Standard septum material is Teflon-coated silicone. Other bottle or septum arrangements are available.

[sentry-equip.com](http://sentry-equip.com)

966 Blue Ribbon Circle North, Oconomowoc, WI 53066 U.S.A. | +1-262-567-7256 | sales@sentry-equip.com

© 2018 Sentry Equipment Corp. All rights reserved. Sentry is a registered trademark of Sentry Equipment Corp. Viton is a registered trademark of The Chemours Company. Kalrez is a registered trademark of E.I. du Pont de Nemours and Company. It is solely the responsibility of end users, through their own testing and analysis, to select products and materials suitable for their specific application requirements, ensure they are properly installed, safely applied and properly maintained, and to limit their use to their intended purpose. Improper selection, installation or use may result in personal injury or property damage.

S-MS-SPS-00188-13 07-23



COMPANY WITH  
 QUALITY SYSTEM  
 CERTIFIED BY DNV GL  
 = ISO 9001 =